

Human APOE Sandwich ELISA Kit Datasheet

Please read it entirely before use

Catalogue Number: KE00156

Size: 96T

Sensitivity: 29.4 pg/mL

Range: 78.1-5000 pg/mL

Usage: For the quantitative detection of human APOE concentrations in serum, plasma, cell culture supernatant, urine, saliva and human cerebrospinal fluid.


This product is for research use only and not for use in human or animal therapeutic or diagnostic.

Table of content	page
1. Background	3
2. Principle	3
3. Required Materials	3
4. Kit Components and Storage	4
5. Safety Notes	4
6. Sample Collection and Storage	4
7. Regent Preparation	5
8. Assay Procedure Summary	6
9. Validation Data	7
9.1 Standard curve	7
9.2 Precision	8
9.3 Recovery	8
9.4 Sample values	8
9.5 Sensitivity	9
9.6 Linearity	9
10. References	9

1. Background

APOE (apolipoprotein E) is a plasma protein implicated in lipid metabolism. It is produced predominantly by hepatocytes, macrophages, and neural cells. In the CNS, APOE is the major extracellular lipid carrier and plays a key role in neuronal protection/repair after injury. APOE is polymorphic, with three major alleles: APOE2 (cys112, cys158), APOE3 (cys112, arg158), and APOE4 (arg112, arg158). APOE2 plays a protective role against both Alzheimer's (AD) and heart disease. APOE4 confers a higher risk for atherosclerosis and Alzheimer's disease. Analysis of cerebrospinal fluid (CSF) and plasma APOE protein levels in AD patients had been performed to examine its association with AD pathology. In old age, high plasma APOE levels precede an increase of circulating CRP and strongly associates with cardiovascular mortality.

2. Principle

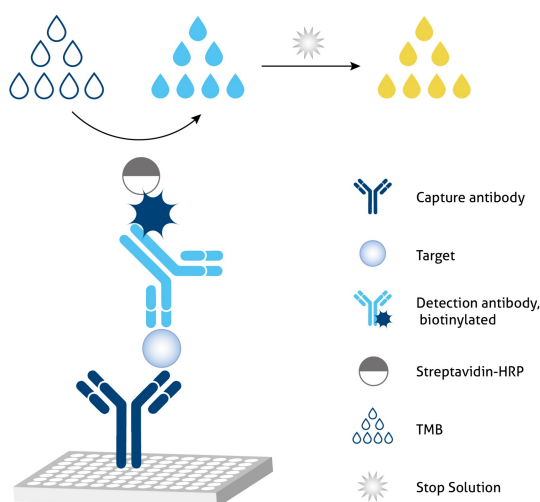

Sandwich ELISA structure (Detection antibody labeled with biotin)

A capture antibody is pre-coated onto the bottom of wells which binds to analyte of interest. A detection antibody labeled with biotin also binds to the analyte. Streptavidin-HRP binds to the biotin. TMB acts as the HRP substrate and the solution color will change from colorless to blue. A stop solution containing sulfuric acid turns solution yellow. The color intensity is proportional to the quantity of bound protein which is measurable at 450 nm with the correction wavelength set at 630 nm.

3. Required Materials

- 3.1 A microplate reader capable of measuring absorbance at 450 nm with the correction wavelength set at 630 nm.
- 3.2 Calibrated, adjustable precision pipettes and disposable plastic tips. A manifold multi-channel pipette is recommended for large assays.
- 3.3 Plate washer: automated or manual.
- 3.4 Absorbent paper towels.
- 3.5 Glass or plastic tubes to prepare standard and sample dilutions.
- 3.6 Beakers and graduated cylinders.
- 3.7 Log-log or semi-log graph paper or computer and software for ELISA data analysis. A four-parameter logistic (4-PL) curve-fit is recommended.

4. Kit Components and Storage

Microplate - antibody coated 96-well microplate (8 well × 12 strips)	1 plate	Unopened Kit: Store at 2-8°C for 6 months or -20°C for 12 months. Opened Kit: All reagents stored at 2-8°C for 7 days. Please use a new standard for each assay.
Protein standard - 10000 pg/bottle; lyophilized	2 bottles	
Detection antibody, biotinylated (100×) - 120 µL/vial*	1 vial	
Streptavidin-horseradish peroxidase (HRP) (100×) - 120 µL/vial*	1 vial	
Sample Diluent PT 4 - 30 mL/bottle. For human serum, plasma, urine and human cerebrospinal fluid samples	2 bottles	
Sample Diluent PT 1 - 30 mL/bottle. For cell culture supernatant and saliva samples	1 bottle	
Detection Diluent - 30 mL/bottle	1 bottle	
Wash Buffer Concentrate (20×) - 30 mL/bottle	1 bottle	
Tetramethylbenzidine Substrate (TMB) - 12 mL/bottle	1 bottle	
Stop Solution - 12 mL/bottle	1 bottle	
Plate Cover Seals	4 pieces	

* Centrifugation immediately before use

5. Safety Notes

5.1 Avoid any skin and eye contact with Stop Solution and TMB. In case of contact, wash thoroughly with water.

5.2 Do not use the kit after the expiration date.

5.3 Do not mix or substitute reagents or materials from other kit lots or other sources.

5.4 Be sure to wear protective equipment such as gloves, masks and goggles during the experiment.

5.5 When using an automated plate washer, adding a 30 second soak period following the addition of Wash Buffer to improve assay precision

6. Sample Collection and Storage

6.1 Serum: Allow blood samples to clot for 30 minutes, followed by centrifugation for 15 minutes at 1000×g. Clear serum can be assayed immediately or aliquoted and stored at -20°C. Avoid repeated freeze-thaw cycles.

6.2 Plasma: Use EDTA, heparin, or citrate as an anticoagulant for plasma collection. Centrifuge for 15 minutes at 1000×g within 30 minutes of collection. The plasma can be assayed immediately or aliquoted and stored at -20°C. Avoid repeated freeze-thaw cycles.

6.3 Cell Culture Supernatant: Remove particulates by centrifugation for 5 minutes at 500×g and assay immediately or aliquot and store samples at ≤ -20°C. Avoid repeated freeze-thaw cycles.

6.4 Urine: Collect urine samples and centrifuge for 20 minutes at 1000×g. Collect the aqueous layer, assay immediately or aliquot and store samples at ≤ -20°C. Avoid repeated freeze-thaw cycles.

6.5 Saliva: Collect saliva samples and centrifuge for 5 minutes at 10,000×g. Collect the aqueous layer, assay immediately or aliquot and store samples at ≤ -20°C. Avoid repeated freeze-thaw cycles.

6.6 Human Cerebrospinal Fluid (CSF): Collect CSF samples in a tube and centrifuge for 15 minutes at 1000×g. Collect the aqueous layer, assay immediately or aliquot and store samples at ≤ -20°C. Avoid repeated freeze-thaw cycles.

7. Regent Preparation

7.1 Wash Buffer (1X): If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Add 30 mL of Wash Buffer Concentrate(20X) to 570 mL deionized or distilled water to prepare 1X Wash Buffer.

7.2 Detection Antibody (1X): Dilute 100X Detection Antibody 1:100 using Detection Diluent prior to assay. Suggested 1:100 dilution: 10 µL 100X Detection Antibody + 990 µL Detection Diluent (Centrifuge the 100 X Detection Antibody solution for a few seconds prior to use).


7.3 Streptavidin-HRP (1X): Dilute 100X Streptavidin-HRP 1:100 using Detection Diluent prior to assay. Suggested 1:100 dilution: 10 µL 100X Streptavidin-HRP + 990 µL Detection Diluent (Centrifuge the 100X Streptavidin-HRP solution for a few seconds prior to use).

7.4 Sample Dilution: Different samples should be diluted with corresponding Sample Diluent, samples may require further dilution if the readout values are higher than the highest standard OD reading. Variations in sample collection, processing and storage may affect the results of the measurement.

Recommended Dilution for different sample types: 1:16,000 or 1:32,000 is recommended for human serum and human plasma; 1:4 or 1:8 is recommended for urine and saliva; 1:800 or 1:1600 is recommended for human cerebrospinal fluid(SCF).

7.5 Standard Serial Dilution:

For human serum, human plasma, urine and human cerebrospinal fluid samples , add 2 mL Sample Diluent PT 4 in protein standard; For saliva samples, add 2 mL Sample Diluent PT 1 in protein standard.

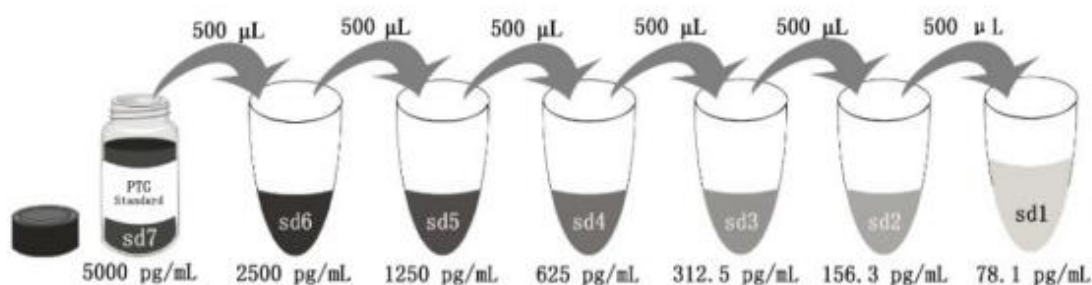

Add # µL of Standard diluted in the previous step	—	500 µL	500 µL	500 µL	500 µL	500 µL	500 µL
# µL of Sample Diluent PT4 or PT 1	2000 µL	500 µL	500 µL	500 µL	500 µL	500 µL	500 µL
	"sd7"	"sd6"	"sd5"	"sd4"	"sd3"	"sd2"	"sd1"

8. Assay Procedure Summary

Bring all reagents to room temperature before use (Detection antibody and Streptavidin-HRP can be used immediately). To avoid cross-contamination, change pipette tips between additions of each standard level, between sample additions, and between reagent additions. Also, use separate reservoirs for each reagent.

8.1 Take out the required number of microplate strips and return excess strips to the foil pouch containing the drying reagent pack and reseal; store at 4°C immediately. Microplate strips should be used in one week.

8.2 Preset the layout of the microplate, including control group, standard group and sample group, add 100 µL of each standard and sample to the appropriate wells. (Make sure sample addition is uninterrupted and completed within 5 to 10 minutes, It is recommended to assay all standards, controls, and samples in duplicate).

8.3 Seal plate with cover seal, pressing it firmly onto top of microwells. Incubate the plate for 2 hours at 37°C.

8.4 Wash

1) Gently remove the cover seal. Discard the liquid from wells by aspirating or decanting. Remove any residual solution by tapping the plate a few times on fresh paper towels.

2) Wash 4 times with 1X Wash Buffer, using at least 350-400 µL per well. Following the last wash, firmly tap plates on fresh towels 10 times to remove residual Wash Buffer. Avoid getting any towel fibers in the wells or wells drying out completely.

8.5 Add 100 µL of 1X Detection Antibody solution (refer to Reagent Preparation 7.2) to each well. Seal plate with cover seal and incubate for 1 hour at 37°C.

8.6 Repeat wash step in 8.4.

8.7 Add 100 µL of 1X Streptavidin-HRP solution (refer to Reagent Preparation 7.3) to each well. Seal plate with cover seal and incubate the plate for 40 minutes at 37°C.

8.8 Repeat wash step in 8.4.

8.9 Signal development: Add 100 µL of TMB substrate solution to each well, protected from light. Incubate for 15 to 20 minutes. Substrate Solution should remain colorless until added to the plate.

8.10 Quenching color development: Add 100 µL of Stop Solution to each well in the same order as addition of the TMB substrate. Mix by tapping the side of the plate gently. NB: Avoid skin and eye contact with the Stop solution.

8.11 Read results: Immediately after adding Stop solution read the absorbance on a microplate reader at a wavelength of 450 nm. If possible, perform a double wavelength readout (450 nm and 630 nm).


8.12 Data analysis: Calculate the average of the duplicate readings (OD value) for each standard and sample, and subtract the average of the zero standard absorbance. Construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis, use four-parameter logistic curve-fit (4-PL) analysis to do this. If the samples have been diluted, the OD readout from the standard curve must be multiplied by the dilution factor used.

Step	Reagent	Volume	Incubation	Wash	Notes
1	Standard and Samples	100 µL	120 min	4 times	Cover Wells incubate at 37°C
2	Diluent Antibody Solution	100 µL	60 min	4 times	Cover Wells incubate at 37°C
3	Diluent HRP Solution	100 µL	40 min	4 times	Cover Wells incubate at 37°C
4	TMB Substrate	100 µL	15-20 min	Do not wash	Incubate in the dark at 37°C
5	Stop Solution	100 µL	0 min	Do not wash	-
6	Read plate at 450 nm and 630 nm immediately after adding Stop solution. DO NOT exceed 5 minutes.				


9. Validation Data

9.1 Standard curve

These standard curves are provided for demonstration only. A standard curve should be generated for each set of samples assayed.

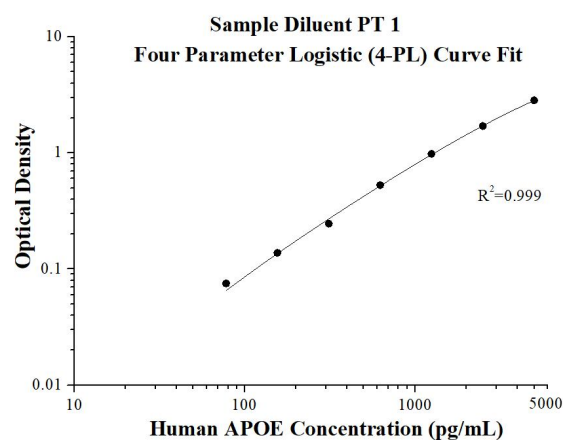

(pg/mL)	O.D	Average	Corrected
0	0.045 0.047	0.046	-
78.1	0.123 0.119	0.121	0.075
156.3	0.183 0.184	0.183	0.137
312.5	0.294 0.289	0.291	0.245
625	0.590 0.558	0.574	0.528
1250	1.019 1.033	1.026	0.980
2500	1.722 1.777	1.749	1.703
5000	2.852 2.905	2.878	2.832

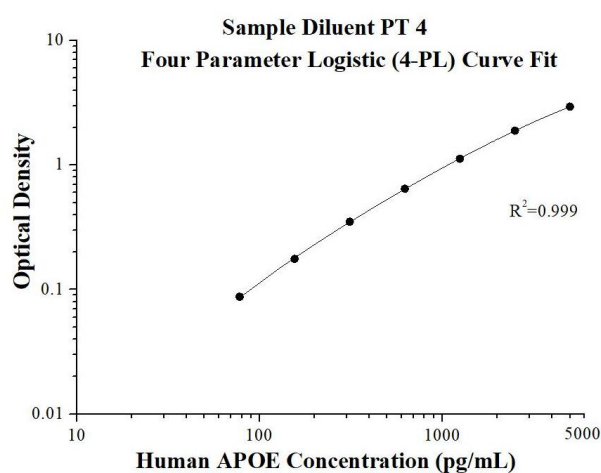

(pg/mL)	O.D	Average	Corrected
0	0.03 0.029	0.029	-
78.1	0.102 0.132	0.117	0.087
156.3	0.191 0.22	0.205	0.176
312.5	0.358 0.402	0.38	0.350
625	0.641 0.706	0.673	0.644
1250	1.166 1.143	1.154	1.125
2500	1.923 1.915	1.919	1.889
5000	2.99 2.954	2.972	2.942

9.2 Precision

Intra-assay Precision (Precision within an assay) Three samples of known concentration were tested 20 times on one plate to assess intra-assay precision.

Inter-assay Precision (Precision between assays) Three samples of known concentration were tested in 24 separate assays to assess inter-assay precision.

Intra-assay Precision					Inter-assay Precision				
Sample	n	Mean (pg/mL)	SD	CV%	Sample	n	Mean (pg/mL)	SD	CV%
1	20	2,811.2	88.6	3.2	1	24	2,846.8	200.8	7.1
2	20	776.0	23.9	3.1	2	24	729.6	22.3	3.1
3	20	291.0	7.4	2.5	3	24	283.9	11.1	3.9

9.3 Recovery

The recovery of human APOE spiked to three different levels throughout the range of the assay in various matrices was evaluated.

Sample Type		Average% of Expected	Range (%)
Human serum	1:32,000	105	87-118
	1:64,000	95	81-116
Saliva	1:8	99	77-125
	1:16	111	97-125
Urine	1:8	116	109-123
	1:16	111	99-118
Human cerebrospinal fluid	1:3,200	76	73-79
	1:6,400	85	75-96

9.4 Sample values

Samples from healthy volunteers were evaluated for human APOE in this assay. No medical histories were available for the donors used in this study.

Sample Type	Mean of Detectable(ng/mL)	Range (ng/mL)
Human serum (n=16)	26,155	8,013-43,244
Human plasma (n=16)	22,498	9,489-65,868
Saliva (n=8)	3.59	1.15-7.03
Urine (n=8)	2.19	0.47-4.54
Human cerebrospinal fluid (n=1)	2,508	-

9.5 Sensitivity

The minimum detectable dose of human APOE is 29.4 pg/mL. This was determined by adding two standard deviations to the concentration corresponding to the mean O.D. of 20 zero standard replicates.

9.6 Linearity

To assess the linearity of the assay, samples were diluted with the appropriate **Sample Diluent** to produce samples with values within the dynamic range of the assay.

(The serum were initially diluted 1:4,000. Human cerebrospinal fluid were initially diluted 1:200)

		Human serum (Sample Diluent PT 4)	Saliva (Sample Diluent PT 1)	Urine (Sample Diluent PT 4)	Human cerebrospinal fluid (Sample Diluent PT 4)
1:2	Average% of Expected	100	-	-	100
	Range (%)	-	-	-	-
1:4	Average% of Expected	96	100	100	99
	Range (%)	94-96	-	-	85-129
1:8	Average% of Expected	88	107	108	105
	Range (%)	79-95	94-118	102-113	93-126
1:16	Average% of Expected	93	109	116	95
	Range (%)	90-98	96-116	108-123	86-102

10. References

1. Teng E. et al. (2015). Dement Geriatr Cogn Disord. 39(3-4):154-66.
2. Mooijaart SP. et al. (2006). PLoS Med. Jun;3(6):e176.