

Human IL-12 p40 Sandwich ELISA Kit Datasheet

Please read it entirely before use

Catalogue Number: KE00240

Size: 96T

Sensitivity: 0.47 pg/mL

Range: 31.25-2000 pg/mL

Usage: For the quantitative detection of human IL-12 p40 concentrations in serum, plasma, cell culture supernatant and urine.


This product is for research use only and not for use in human or animal therapeutic or diagnostic.

Table of content	page
1. Background	3
2. Principle	3
3. Required Materials	3
4. Kit Components and Storage	4
5. Safety Notes	4
6. Sample Collection and Storage	4
7. Regent Preparation	5
8. Assay Procedure Summary	6
9. Validation Data	6
9.1 Standard curve	6
9.2 Precision	8
9.3 Recovery	8
9.4 Sample values	9
9.5 Sensitivity	9
9.6 Linearity	10
10. References	10

1. Background

Interleukin-12 (IL-12), is a cytokine that is secreted by activated phagocytes and dendritic cells and that induces interferon- γ production by natural-killer and T lymphocytes. IL-12 is a 75 kDa heterodimer composed of a 35 kDa subunit (IL-12A p35) and a 40 kDa subunit (IL-12B p40) that is secreted by a wide variety of antigen presenting cells (APCs), including phagocytes, B cells and Langerhans cells. IL-12 p40 has been found to be important for sustaining a sufficient number of memory/effector Th1 cells to mediate long-term protection to an intracellular pathogen. Overexpression of IL-12 p40 was observed in the central nervous system of patients with multiple sclerosis (MS), suggesting a role of this cytokine in the pathogenesis of the disease. The promoter polymorphism of IL-12 p40 has been reported to be associated with the severity of atopic and non-atopic asthma in children.

2. Principle

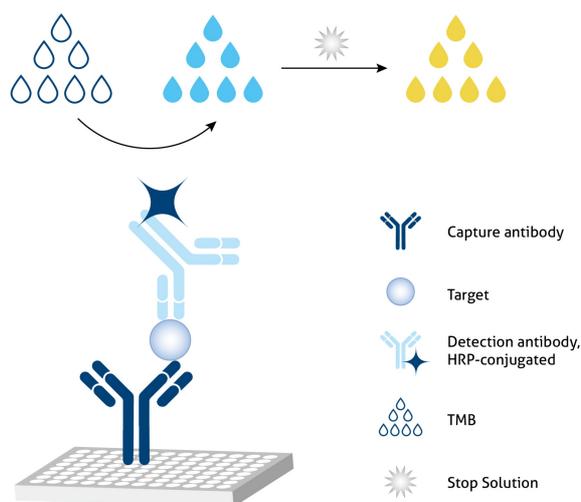

Sandwich ELISA structure (Detection antibody labeled with HRP)

A capture antibody is pre-coated onto the bottom of wells which binds to analyte of interest. A detection antibody labeled with HRP also binds to the analyte. TMB acts as the HRP substrate and the solution color will change from colorless to blue. A stop solution containing sulfuric acid turns solution yellow. The color intensity is proportional to the quantity of bound protein which is measurable at 450 nm with the correction wavelength set at 630 nm.

3. Required Materials

- 3.1 A microplate reader capable of measuring absorbance at 450 nm with the correction wavelength set at 630 nm.
- 3.2 Calibrated, adjustable precision pipettes and disposable plastic tips. A manifold multi-channel pipette is recommended for large assays.
- 3.3 Plate washer: automated or manual.
- 3.4 Absorbent paper towels.
- 3.5 Glass or plastic tubes to prepare standard and sample dilutions.
- 3.6 Beakers and graduated cylinders.
- 3.7 Log-log or semi-log graph paper or computer and software for ELISA data analysis. A four-parameter logistic (4-PL) curve-fit is recommended.

4. Kit Components and Storage

Microplate - antibody coated 96-well microplate (8 well × 12 strips)	1 plate	Unopened Kit: Store at 2-8°C for 6 months or -20°C for 12 months. Opened Kit: All reagents stored at 2-8°C for 7 days. Please use a new standard for each assay.
Protein standard - 2000 pg/bottle; lyophilized	2 bottles	
Detection antibody, HRP-conjugated (100×) - 120 µL/vial*	1 vial	
Sample Diluent PT 3 - 30 mL/bottle. For human serum and plasma	1 bottle	
Sample Diluent PT 1-ef - 30 mL/bottle. For cell culture supernatant	1 bottle	
Sample Diluent PT 1 - 30 mL/bottle. For urine	1 bottle	
Detection Diluent - 30 mL/bottle	1 bottle	
Wash Buffer Concentrate (20×) - 30 mL/bottle	1 bottle	
Tetramethylbenzidine Substrate (TMB) - 12 mL/bottle	1 bottle	
Stop Solution - 12 mL/bottle	1 bottle	
Plate Cover Seals	4 pieces	

* Centrifugation immediately before use

5. Safety Notes

- 5.1 Avoid any skin and eye contact with Stop Solution and TMB. In case of contact, wash thoroughly with water.
- 5.2 Do not use the kit after the expiration date.
- 5.3 Do not mix or substitute reagents or materials from other kit lots or other sources.
- 5.4 Be sure to wear protective equipment such as gloves, masks and goggles during the experiment.
- 5.5 When using an automated plate washer, adding a 30 second soak period following the addition of Wash Buffer to improve assay precision

6. Sample Collection and Storage

- 6.1 Serum: Allow blood samples to clot for 30 minutes, followed by centrifugation for 15 minutes at 1000xg. Clear serum can be assayed immediately or aliquoted and stored at -20°C. Avoid repeated freeze-thaw cycles.
- 6.2 Plasma: Use EDTA, heparin, or citrate as an anticoagulant for plasma collection. Centrifuge for 15 minutes at 1000xg within 30 minutes of collection. The plasma can be assayed immediately or aliquoted and stored at -20°C. Avoid repeated freeze-thaw cycles.
- 6.3 Cell Culture Supernatant: Remove particulates by centrifugation for 5 minutes at 500xg and assay immediately or aliquot and store samples at ≤ -20°C. Avoid repeated freeze-thaw cycles.
- 6.4 Urine: Collect urine samples and centrifuge for 20 minutes at 1000xg. Collect the aqueous layer, assay immediately or aliquot and store samples at ≤ -20°C. Avoid repeated freeze-thaw cycles.

7. Regent Preparation

7.1 Wash Buffer (1X): If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Add 30 mL of Wash Buffer Concentrate(20X) to 570 mL deionized or distilled water to prepare 1X Wash Buffer.


7.2 Detection Antibody, HRP-conjugated (1X): Dilute 100X Detection Antibody, HRP-conjugated 1:100 using Detection Diluent prior to assay. Suggested 1:100 dilution: 10 μ L 100X Detection Antibody, HRP-conjugated + 990 μ L Detection Diluent (Centrifuge the 100 X Detection Antibody solution, HRP-conjugated for a few seconds prior to use)

7.3 Sample Dilution: Different samples should be diluted with corresponding Sample Diluent, samples may require further dilution if the readout values are higher than the highest standard OD reading. Variations in sample collection, processing and storage may affect the results of the measurement.

Recommended Dilution for different sample types: 1:2 or 1:4 is recommended for human serum and plasma; 1:2 or 1:4 is recommended for cell culture supernatant.

7.4 Standard Serial Dilution:

For human serum and plasma samples, add 1 mL Sample Diluent PT 3 in protein standard; For cell culture supernatant sample, add 1 mL Sample Diluent PT 1-ef in protein standard; For urine sample, add 1 mL Sample Diluent PT 1 in protein standard.

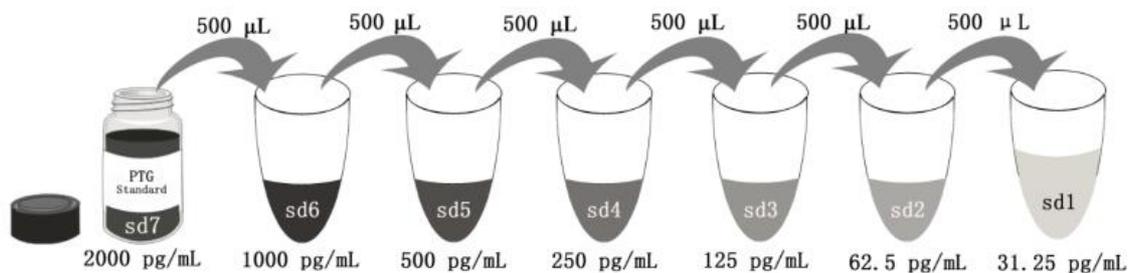

Add # μ L of Standard diluted in the previous step	—	500 μ L					
# μ L of Sample Diluent PT 3,PT 1-ef or PT 1	1000 μ L	500 μ L					
	"sd7"	"sd6"	"sd5"	"sd4"	"sd3"	"sd2"	"sd1"

8. Assay Procedure Summary

Bring all reagents to room temperature before use (Detection antibody, HRP-conjugated can be used immediately). To avoid cross-contamination, change pipette tips between additions of each standard level, between sample additions, and between reagent additions. Also, use separate reservoirs for each reagent.

8.1 Take out the required number of microplate strips and return excess strips to the foil pouch containing the drying reagent pack and reseal; store at 4°C immediately. Microplate strips should be used in one week.

8.2 Preset the layout of the microplate, including control group, standard group and sample group, add 100 µL of each standard and sample to the appropriate wells. (Make sure sample addition is uninterrupted and completed within 5 to 10 minutes, it is recommended to assay all standards, controls, and samples in duplicate).

8.3 Seal plate with cover seal, pressing it firmly onto top of microwells. Incubate the plate for 2 hours at 37°C.

8.4 Wash

1) Gently remove the cover seal. Discard the liquid from wells by aspirating or decanting. Remove any residual solution by tapping the plate a few times on fresh paper towels.

2) Wash 4 times with 1X Wash Buffer, using at least 350-400 µL per well. Following the last wash, firmly tap plates on fresh towels 10 times to remove residual Wash Buffer. Avoid getting any towel fibers in the wells or wells drying out completely.

8.5 Add 100 µL of 1X Detection antibody, HRP-conjugated solution (refer to Reagent Preparation 7.2) to each well. Seal plate with cover seal and incubate for 40 minutes at 37°C.

8.6 Repeat wash step in 8.4.

8.7 Signal development: Add 100 µL of TMB substrate solution to each well, protected from light. Incubate for 15 to 20 minutes. Substrate Solution should remain colorless until added to the plate.

8.8 Quenching color development: Add 100 µL of Stop Solution to each well in the same order as addition of the TMB substrate. Mix by tapping the side of the plate gently. NB: Avoid skin and eye contact with the Stop solution.

8.9 Read results: Immediately after adding Stop solution read the absorbance on a microplate reader at a wavelength of 450 nm. If possible, perform a double wavelength readout (450 nm and 630 nm).

8.10 Data analysis: Calculate the average of the duplicate readings (OD value) for each standard and sample, and subtract the average of the zero standard absorbance. Construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis, use four-parameter logistic curve-fit (4-PL) analysis to do this. If the samples have been diluted, the OD readout from the standard curve must be multiplied by the dilution factor used.


Step	Reagent	Volume	Incubation	Wash	Notes
1	Standard and Samples	100 µL	120 min	4 times	Cover Wells incubate at 37°C
2	Diluent Detection antibody, HRP-conjugated Solution	100 µL	40 min	4 times	Cover Wells incubate at 37°C
3	TMB Substrate	100 µL	15-20 min	Do not wash	Incubate in the dark at 37°C
4	Stop Solution	100 µL	0 min	Do not wash	-
5	Read plate at 450 nm and 630 nm immediately after adding Stop solution. DO NOT exceed 5 minutes.				

9. Validation Data


9.1 Standard curve

These standard curves are provided for demonstration only. A standard curve should be generated for each set of samples


assayed.

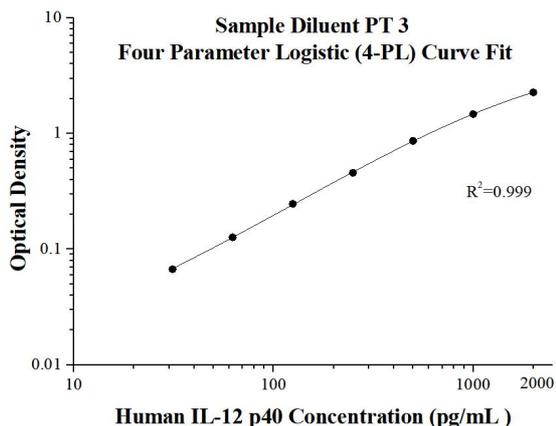

(pg/mL)	O.D	Average	Corrected
0	0.062 0.062	0.062	-
31.25	0.113 0.113	0.113	0.051
62.5	0.165 0.165	0.165	0.103
125	0.269 0.27	0.2695	0.2075
250	0.466 0.471	0.4685	0.4065
500	0.822 0.829	0.8255	0.7635
1000	1.414 1.443	1.4285	1.3665
2000	2.267 2.326	2.2965	2.2345

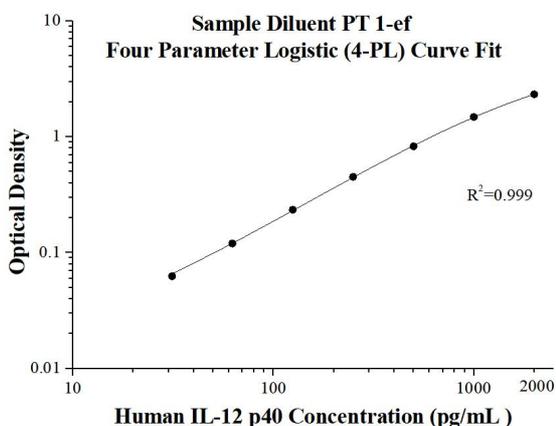

(pg/mL)	O.D	Average	Corrected
0	0.055 0.057	0.056	-
31.25	0.117 0.12	0.1185	0.0625
62.5	0.176 0.176	0.176	0.12
125	0.287 0.294	0.2905	0.2345
250	0.499 0.518	0.5085	0.4525
500	0.862 0.905	0.8835	0.8275
1000	1.508 1.567	1.5375	1.4815
2000	2.355 2.418	2.3865	2.3305

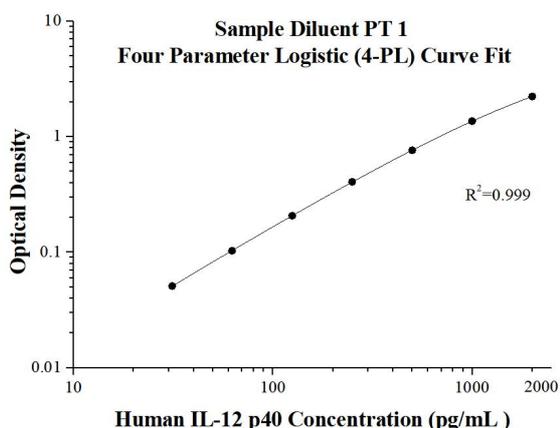

(pg/mL)	O.D	Average	Corrected
0	0.067 0.066	0.0665	-
31.25	0.132 0.135	0.1335	0.067
62.5	0.191 0.195	0.193	0.1265
125	0.31 0.316	0.313	0.2465
250	0.523 0.526	0.5245	0.458
500	0.919 0.943	0.931	0.8645
1000	1.521 1.561	1.541	1.4745
2000	2.354 2.322	2.338	2.2715

9.2 Precision

Intra-assay Precision (Precision within an assay) Three samples of known concentration were tested 20 times on one plate to assess intra-assay precision.

Inter-assay Precision (Precision between assays) Three samples of known concentration were tested in 24 separate assays to assess inter-assay precision.

Intra-assay Precision					Inter-assay Precision				
Sample	n	Mean (pg/mL)	SD	CV%	Sample	n	Mean (pg/mL)	SD	CV%
1	20	965.3	20.8	2.2	1	24	953.9	33.7	3.5
2	20	209.6	3.4	1.6	2	24	202.0	6.4	3.2
3	20	49.8	1.5	3.1	3	24	48.7	2.0	4.0

9.3 Recovery

The recovery of human IL-12 p40 spiked to three different levels throughout the range of the assay in various matrices was evaluated.

Sample Type		Average% of Expected	Range (%)
Human plasma	1:2	88	84-96
	1:4	96	80-121
Cell culture supernatant	1:4	108	101-126
	1:8	100	92-111
Urine	1:2	94	85-110
	1:4	95	85-103

9.4 Sample values

Human serum/plasma -eight human serum and eight human plasma samples from healthy volunteers were evaluated for human IL-12 p40 in this assay. No medical histories were available for the donors used in this study.

Sample Type	Mean (pg/mL)	Range (pg/mL)
Human serum (n=8)	195.5	91.7-274.4
Human plasma (n=8)	135.4	75.9-254.8

Urine -Five urine samples from healthy volunteers were evaluated for human IL-12 p40 in this assay. All samples measured less than the lowest standard, 31.25 pg/mL. No medical histories were available for the donors used in this study.

Cell culture supernatant - Human peripheral blood mononuclear cells (1×10^6 cells/mL in RPMI 1640 supplemented with 5%FBS) were cultured overnight with or without 100ng/mL recombinant human IFN-gamma(Catalogo No.: HZ-1301) and then 24 hours with or without addition of 10ug/mL LPS. Aliquots of the cell culture supernatant was removed and assayed for levels of human IL-12 p40.

Condition	(pg/mL)
Unstimulated for 1d	-
Stimulated for 1d	2,767.0

9.5 Sensitivity

The minimum detectable dose of human IL-12 p40 is 0.47 pg/mL. This was determined by adding two standard deviations to the concentration corresponding to the mean O.D. of 20 zero standard replicates.

9.6 Linearity

To assess the linearity of the assay, human plasma and urine samples were spiked with high concentrations of human IL-12 p40 and diluted with the appropriate **Sample Diluent** to produce samples with values within the dynamic range of the assay. Cell culture supernatant was diluted with the appropriate **Sample Diluent** to produce samples with values within the dynamic range of the assay.

Sample Type		Range (%)	Average% of Expected
Human plasma (Sample Diluent PT 3)	1:2	84-91	88
	1:4	90-98	95
	1:8	98-105	101
	1:16	103-117	108
Cell culture supernatant (Sample Diluent PT 1-ef)	1:2	-	100
	1:4	97-100	99
	1:8	100-102	101
	1:16	99-104	102
Urine (Sample Diluent PT 1)	1:2	92-95	93
	1:4	93-98	96
	1:8	96-105	99
	1:16	103-113	109

10. References

1. Cooper AM. et al. (2007) Trends Immunol. 28:33-8.
2. Wang SZ. et al. (2004) J Immunol. 173:4040-9.
3. Bielekova B. et al. (2012) PLoS One. 7:e48370.
4. Xu J. et al. (2016) Cell Death Differ. 23:1941-1951.