

Speedy™ Human/Cynomolgus Monkey IgG One-Step ELISA Kit Datasheet

Please read it entirely before use

Catalogue Number: SE50326

Size: 96T

Sensitivity: 0.02 ng/mL

Range: 0.156-10 ng/mL

Usage: For the quantitative detection of human/cynomolgus monkey IgG concentrations in serum, plasma, urine, saliva and human milk.


This product is for research use only and not for use in human or animal therapeutic or diagnostic.

Table of content	page
1. Background	3
2. Principle	3
3. Required Materials	3
4. Kit Components and Storage	4
5. Safety Notes	4
6. Sample Collection and Storage	4
7. Regent Preparation	5
8. Assay Procedure Summary	6
9. Validation Data	7
9.1 Standard curve	7
9.2 Precision	8
9.3 Recovery	8
9.4 Sample values	9
9.5 Sensitivity	9
9.6 Linearity	10
9.7 Specificity	11
10. References	11

1. Background

Immunoglobulin G (IgG) is the most abundant antibody isotype in human serum. It is a monomeric glycoprotein composed of two identical heavy chains and two identical light chains, with a molecular weight of about 150 kDa. IgG plays a central role in adaptive immunity by mediating pathogen neutralization, opsonization, and complement activation. Its four subclasses (IgG1, IgG2, IgG3, and IgG4) exhibit distinct functional profiles and differential affinities for Fc receptors, enabling tailored immune responses. Notably, IgG is the only antibody class capable of crossing the placental barrier, providing passive immunity to newborns.

2. Principle

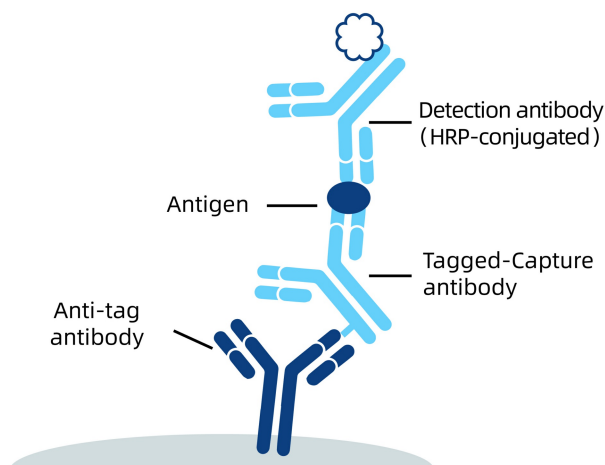

An anti-tag antibody is pre-coated onto the bottom of wells. After adding antigen or samples, Tagged-Capture antibody and HRP-conjugated detection antibody, a sandwich complex is formed in the solution. TMB acts as a HRP substrate, and the solution color will change from colorless to blue. A stop solution containing sulfuric acid turns the solution yellow. The color intensity is proportional to the quantity of bound protein, which is measurable at 450 nm with the correction wavelength set at 630 nm.

3. Required Materials

- 3.1 A microplate reader capable of measuring absorbance at 450 nm with the correction wavelength set at 630 nm.
- 3.2 Calibrated, adjustable precision pipettes and disposable plastic tips. A manifold multi-channel pipette is recommended for large assays.
- 3.3 Plate washer: automated or manual.
- 3.4 Absorbent paper towels.
- 3.5 Glass or plastic tubes to prepare standard and sample dilutions.
- 3.6 Beakers and graduated cylinders.
- 3.7 Log-log or semi-log graph paper or computer and software for ELISA data analysis. A four-parameter logistic (4-PL) curve-fit is recommended. Proteintech data analysis website, <https://www.ptgcn.com/products/elisa-kits/>.
- 3.8 Microplate thermostatic shaker.

4. Kit Components and Storage

Microplate - 96 well microplate precoated an anti-tag antibody (8 well × 12 strips)	1 plate	Unopened Kit: Store at 2-8°C for 6 months or -20°C for 12 months. Opened Kit: All reagents stored at 2-8°C for 7 days. Please use a new standard for each assay.
Protein standard - 20 ng/bottle; lyophilized	2 bottles	
Capture Antibody (100×) - 60 uL/vial*	1 vial	
Detection antibody, HRP-Conjugated (100×) - 60 uL/vial*	1 vial	
Sample Diluent PT 4B1 - 30 mL/bottle	3 bottles	
Detection Diluent PT PB1 - 15 mL/bottle	1 bottle	
Wash Buffer Concentrate (20×) - 30 mL/bottle	1 bottle	
Tetramethylbenzidine Substrate (TMB) - 12 mL/bottle	1 bottle	
Stop Solution - 12 mL/bottle	1 bottle	
Plate Cover Seals	4 pieces	

* Centrifugation immediately before use

5. Safety Notes

- 5.1 Avoid any skin and eye contact with Stop Solution and TMB. In case of contact, wash thoroughly with water.
- 5.2 Do not use the kit after the expiration date.
- 5.3 Do not mix or substitute reagents or materials from other kit lots or other sources.
- 5.4 Be sure to wear protective equipment such as gloves, masks and goggles during the experiment.
- 5.5 When using an automated plate washer, adding a 30 second soak period following the addition of Wash Buffer to improve assay precision

6. Sample Collection and Storage

- 6.1 Serum: Allow blood samples to clot for 30 minutes, followed by centrifugation for 15 minutes at 1000xg. Clear serum can be assayed immediately or aliquoted and stored at -20°C. Avoid repeated freeze-thaw cycles.
- 6.2 Plasma: Use EDTA, heparin, or citrate as an anticoagulant for plasma collection. Centrifuge for 15 minutes at 1000xg within 30 minutes of collection. The plasma can be assayed immediately or aliquoted and stored at -20°C. Avoid repeated freeze-thaw cycles.
- 6.3 Urine: Collect urine samples and centrifuge for 20 minutes at 1000xg. Collect the aqueous layer, assay immediately or aliquot and store samples at ≤ -20°C. Avoid repeated freeze-thaw cycles.
- 6.4 Saliva: Collect saliva samples and centrifuge for 5 minutes at 10,000xg. Collect the aqueous layer, assay immediately or aliquot and store samples at ≤ -20°C. Avoid repeated freeze-thaw cycles.
- 6.5 Human Milk: Collect milk samples and Centrifuge for 15 minutes at 1000xg at 2-8°C. Collect the aqueous fraction and repeat this process a total of 3 times. Assay immediately.

7. Regent Preparation

7.1 Wash Buffer (1X): If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Add 30 mL of Wash Buffer Concentrate(20X) to 570 mL deionized or distilled water to prepare 1X Wash Buffer.

7.2 Antibody Cocktail (1X): Dilute 100X capture antibody and 100X HRP-conjugated detection antibody using Detection Diluent prior to assay. Suggested 1:100 dilution: 50 μ L 100X capture antibody + 50 μ L 100X Detection Antibody, HRP-conjugated + 4,900 μ L Detection Diluent. Mix gently but thoroughly.


7.3 Sample Dilution: Different samples should be diluted with corresponding Sample Diluent. The minimum required dilution factor was 1:2; consequently, no more than 25 μ L of undiluted sample was added per well.

Samples may require further dilution if the readout values are higher than the highest standard OD reading. Variations in sample collection, processing and storage may affect the results of the measurement.

Recommended Dilution for different sample types: 1:4,000,000 or 1:8,000,000 is recommended for human serum and plasma; 1:4,000,000 or 1:8,000,000 is recommended for cynomolgus monkey serum and plasma; 1:800 or 1:1,600 is recommended for urine; 1:400 or 1:800 is recommended for saliva; 1:4,000 or 1:8,000 is recommended for human milk.

7.4 Standard Serial Dilution:

Add 2 mL Sample Diluent PT 4B1 in protein standard.

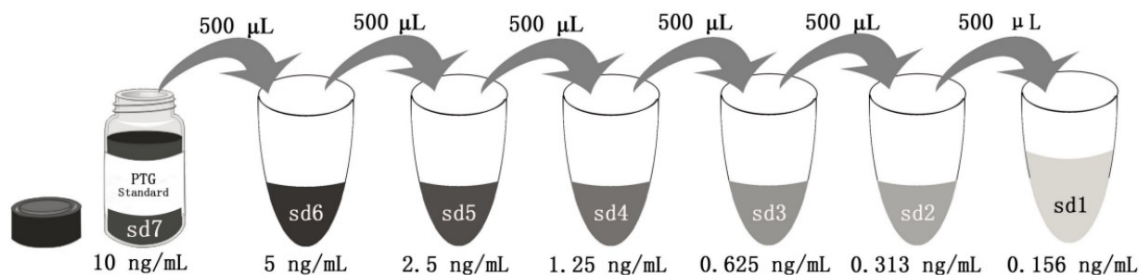

Add # μ L of Standard diluted in the previous step	—	500 μ L	500 μ L	500 μ L	500 μ L	500 μ L	500 μ L
# μ L of Sample Diluent PT 4B1	2000 μ L	500 μ L	500 μ L	500 μ L	500 μ L	500 μ L	500 μ L
	"sd7"	"sd6"	"sd5"	"sd4"	"sd3"	"sd2"	"sd1"

8. Assay Procedure Summary

Bring all reagents to room temperature before use (Detection antibody, HRP-conjugated antibody can be used immediately). To avoid cross-contamination, change pipette tips between additions of each standard level, between sample additions, and between reagent additions. Also, use separate reservoirs for each reagent.

8.1 Preset the layout of the microplate, including control group, standard group and sample group, take out the required number of microplate strips and return excess strips to the foil pouch containing the drying reagent pack and reseal; store at 4°C immediately. Microplate strips should be used in one week.

8.2 Add 50 µL standard or sample to appropriate wells. To avoid high background always add samples or standards to the well before the addition of antibody cocktail.

8.3 Add 50 µL 1× Antibody Cocktail solution (refer to Reagent Preparation 7.2) to each well. Seal plate with cover seal and incubate at 37°C on a microplate thermostatic shaker set at 400 rpm for 1 hour (incubate at 37°C for 2 hours is recommended if thermostatic shaker is not available).

8.4 Wash

1) Gently remove the cover seal. Discard the liquid from wells by aspirating or decanting. Remove any residual solution by tapping the plate a few times on fresh paper towels.

2) Wash 4 times with 1× Wash Buffer, using at least 350-400 µL per well. Following the last wash, firmly tap plates on fresh towels 10 times to remove residual Wash Buffer. Avoid getting any towel fibers in the wells or wells drying out completely.


8.5 Add 100 µL TMB substrate solution to each well, protected from light. Incubate at 37°C on a microplate thermostatic shaker set at 400 rpm for 15 to 20 minutes. (Substrate Solution should remain colorless until added to the plate.)

8.6 Add 100 µL Stop Solution to each well in the same order as addition of the TMB substrate. Note: Avoid skin and eye contact with the Stop solution.

8.7 Read results immediately on a microplate reader at a wavelength of 450 nm. If possible, perform a double wavelength readout (450 nm and 630 nm).

8.8 Data analysis: Calculate the average of the duplicate readings (OD value) for each standard and sample, and subtract the average of the zero standard absorbance. Construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis, four-parameter logistic curve-fit (4-PL) analysis is recommended. If the samples have been diluted, the fitting result must be multiplied by the dilution factor used.


Procedure summary

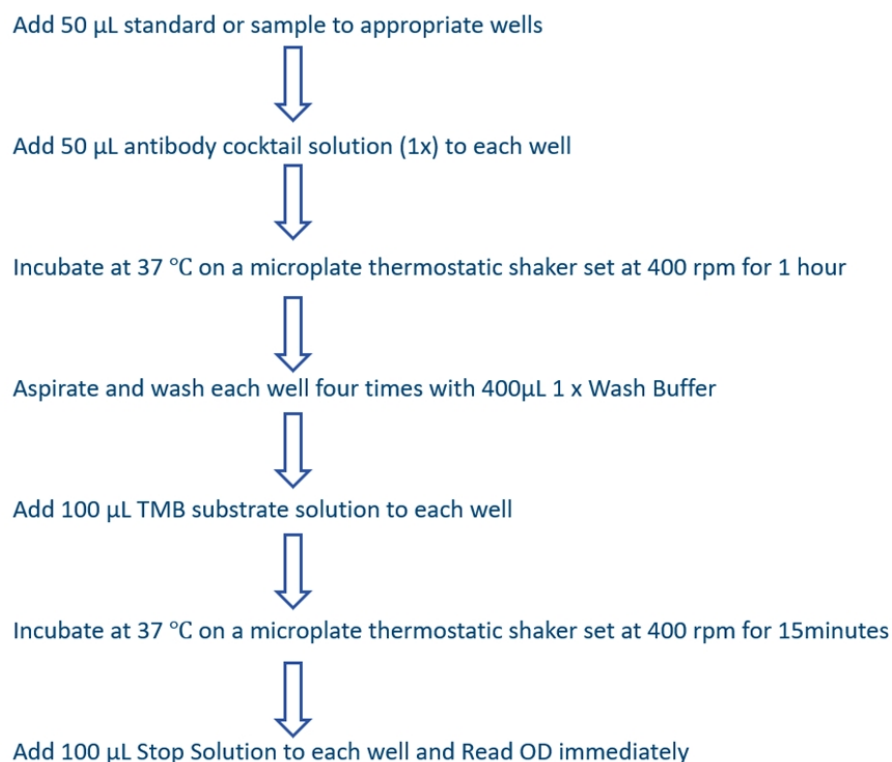

9. Validation Data

9.1 Standard curve

These standard curves are provided for demonstration only. A standard curve should be generated for each set of samples assayed.

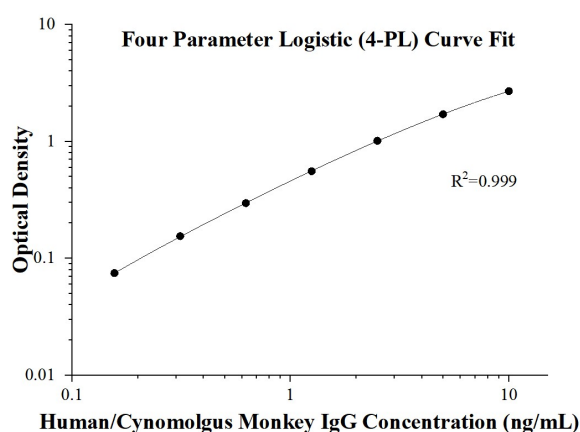

(ng/mL)	O.D	Average	Corrected
0	0.0536 0.0494	0.0515	-
0.156	0.1267 0.1256	0.1262	0.0747
0.313	0.2108 0.2016	0.2062	0.1547
0.625	0.3503 0.3473	0.3488	0.2973
1.25	0.6195 0.596	0.6078	0.5563
2.5	1.0675 1.0632	1.0654	1.0139
5	1.7608 1.7672	1.7640	1.7125
10	2.7393 2.7523	2.7458	2.6943

9.2 Precision

Intra-assay Precision (Precision within an assay) Three samples of known concentration were tested 8 times on one plate to assess intra-assay precision.

Inter-assay Precision (Precision between assays) Three samples of known concentration were tested in 16 separate assays to assess inter-assay precision.

Intra-assay Precision					Inter-assay Precision				
Sample	n	Mean (ng/mL)	SD	CV%	Sample	n	Mean (ng/mL)	SD	CV%
1	8	5.43	0.20	3.68	1	16	5.81	0.58	9.98
2	8	1.16	0.04	3.45	2	16	1.21	0.08	6.61
3	8	0.62	0.05	8.06	3	16	0.63	0.05	7.94

9.3 Recovery

The recovery of human/cynomolgus monkey IgG spiked to three different levels throughout the range of the assay in various matrices was evaluated.

Sample Type		Average% of Expected	Range (%)
Human plasma	1:16,000,000	118	114-124
	1:32,000,000	95	83-103
Cynomolgus monkey serum	1:16,000,000	103	101-104
	1:32,000,000	103	102-105
Human urine	1:3,200	100	96-103
	1:6,400	107	102-116
Human saliva	1:1,600	100	96-105
	1:3,200	96	93-100
Human milk	1:16,000	101	96-109
	1:32,000	99	98-100

9.4 Sample values

Plasma/Serum/Urine/Saliva/Human milk - Plasma, serum, urine, saliva and human milk samples were evaluated for the presence of human/cynomolgus monkey IgG in this assay.

Sample Type	Mean (mg/mL)	Range (mg/mL)
Human plasma (n=16)	10.32	3.49-31.70
Cynomolgus monkey serum (n=11)	14.06	7.91-20.25

Sample Type	Mean (ng/mL)	Range (ng/mL)
Human urine (n=8)	2,002.81	365.91-4,860.26
Human saliva (n=8)	2,236.75	202.17-8,851.72

Sample Type	Mean (ug/mL)	Range (ug/mL)
Human milk (n=8)	12.82	5.53-23.30

9.5 Sensitivity

The minimum detectable dose of human/cynomolgus monkey IgG is 0.02 ng/mL. This was determined by adding two standard deviations to the concentration corresponding to the mean O.D. of 20 zero standard replicates.

9.6 Linearity

To assess the linearity of the assay, samples were diluted with the appropriate **Sample Diluent** to produce samples with values within the dynamic range of the assay.

(The human plasma was initially diluted 1:2,000,000. The cynomolgus monkey serum was initially diluted 1:2,000,000. The human urine was initially diluted 1:400. The human saliva was initially diluted 1:200. The human milk was initially diluted 1:2,000.)

		Human plasma	Cynomolgus monkey serum	Human urine	Human saliva	Human milk
1:2	Average% of Expected	100	100	100	100	100
	Range (%)	-	-	-	-	-
1:4	Average% of Expected	105	105	105	101	89
	Range (%)	104-107	103-106	98-112	98-104	81-97
1:8	Average% of Expected	110	111	110	102	95
	Range (%)	108-112	110-111	107-112	99-105	83-107
1:16	Average% of Expected	112	110	113	104	109
	Range (%)	112-113	108-112	110-117	97-111	96-122

9.7 Specificity

This assay recognizes natural and recombinant human/cynomolgus monkey IgG.

The following factors prepared at 50 ng/mL were assayed and exhibited no cross-reactivity or interference.

Recombinant human:

IgA2

IgE

IgD

IgM

The following factors prepared at 6.25 ng/mL were assayed and exhibited cross-reactivity or interference.


Recombinant human:

IgG1

IgG2

IgG3

IgG4

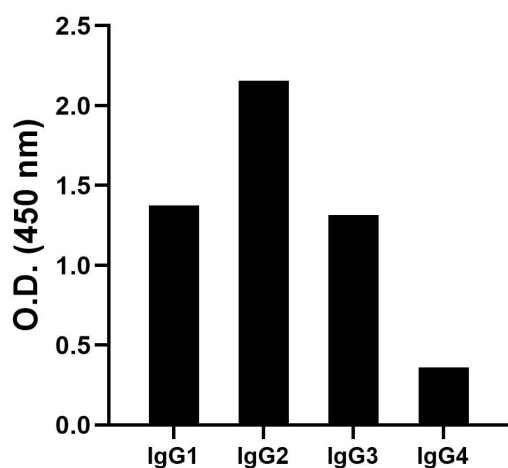

10. References

1. Vidarsson, Gestur et al. *Frontiers in immunology* vol. 5 (2014): 520.
2. Napodano, Cecilia et al. *Immunological investigations* vol. 50,4 (2021): 427-444.
3. Palmeira, Patricia et al. *Clinical & developmental immunology* vol. 2012 (2012): 985646.
4. Krištić, Jasminka, and Gordan Lauc. *Immunological reviews* vol. 328,1 (2024): 143-170.
5. Radovani, Barbara, and Falk Nimmerjahn. *Journal of immunology* (Baltimore, Md. : 1950) vol. 213,11 (2024): 1573-1584.
6. Ma, Hui, and Richard O'Kennedy. *Methods in molecular biology* (Clifton, N.J.) vol. 1348 (2015): 7-11.