

Speedy™ Human/Cynomolgus Monkey MCP-1/CCL2 One-Step ELISA Kit

Datasheet

Please read it entirely before use

Catalogue Number: SE50041

Size: 96T

Sensitivity: 0.5 pg/mL

Range: 3.13-200 pg/mL

Usage: For the quantitative detection of human/cynomolgus monkey MCP-1/CCL2 concentrations in serum, plasma, cell culture supernatant and urine.


This product is for research use only and not for use in human or animal therapeutic or diagnostic.

Table of content	page
1. Background	3
2. Principle	3
3. Required Materials	3
4. Kit Components and Storage	4
5. Safety Notes	4
6. Sample Collection and Storage	4
7. Regent Preparation	5
8. Assay Procedure Summary	6
9. Validation Data	7
9.1 Standard curve	7
9.2 Precision	8
9.3 Recovery	8
9.4 Sample values	9
9.5 Sensitivity	9
9.6 Linearity	10
9.7 Specificity	10
10. References	11

1. Background

Monocyte chemotactic protein 1 (MCP1; also known as CCL2), is a chemokine that can be expressed in monocytes, macrophages, and endothelial cells, and belongs to the CC subfamily of chemokines. Chemokines are a superfamily of secreted proteins involved in immunoregulatory and inflammatory processes. Research has shown that the expression of MCP1 increases in the serum of patients with acute myocarditis. MCP1 is up-regulated in many types of CNS injury, including ischemia, hemorrhage, trauma, infection, hypoxia, and peripheral nerve axotomy. MCP1 has also been implicated in the pathogenesis of diseases characterized by monocytic infiltrates, such as psoriasis, rheumatoid arthritis, and atherosclerosis.

2. Principle

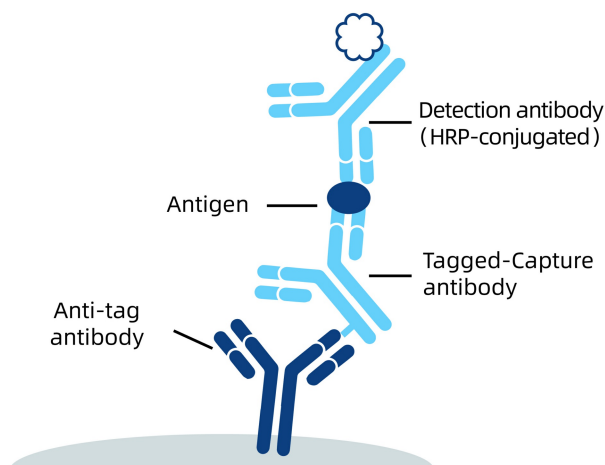

An anti-tag antibody is pre-coated onto the bottom of wells. After adding antigen or samples, Tagged-Capture antibody and HRP-conjugated detection antibody, a sandwich complex is formed in the solution. TMB acts as a HRP substrate, and the solution color will change from colorless to blue. A stop solution containing sulfuric acid turns the solution yellow. The color intensity is proportional to the quantity of bound protein, which is measurable at 450 nm with the correction wavelength set at 630 nm.

3. Required Materials

- 3.1 A microplate reader capable of measuring absorbance at 450 nm with the correction wavelength set at 630 nm.
- 3.2 Calibrated, adjustable precision pipettes and disposable plastic tips. A manifold multi-channel pipette is recommended for large assays.
- 3.3 Plate washer: automated or manual.
- 3.4 Absorbent paper towels.
- 3.5 Glass or plastic tubes to prepare standard and sample dilutions.
- 3.6 Beakers and graduated cylinders.
- 3.7 Log-log or semi-log graph paper or computer and software for ELISA data analysis. A four-parameter logistic (4-PL) curve-fit is recommended. Proteintech data analysis website, <https://www.ptgcn.com/products/elisa-kits/>.
- 3.8 Microplate thermostatic shaker.

4. Kit Components and Storage

Microplate - 96 well microplate precoated an anti-tag antibody (8 well × 12 strips)	1 plate	Unopened Kit: Store at 2-8°C for 6 months or -20°C for 12 months. Opened Kit: All reagents stored at 2-8°C for 7 days. Please use a new standard for each assay.
Protein standard - 400 pg/bottle; lyophilized	2 bottles	
Capture antibody (100×) - 60 uL/vial*	1 vial	
Detection antibody, HRP-Conjugated (100×) - 60 uL/vial*	1 vial	
Sample Diluent PT 3-ef - 30 mL/bottle	1 bottle	
Detection Diluent - 15 mL/bottle	1 bottle	
Wash Buffer Concentrate (20×) - 30 mL/bottle	1 bottle	
Tetramethylbenzidine Substrate (TMB) - 12 mL/bottle	1 bottle	
Stop Solution - 12 mL/bottle	1 bottle	
Plate Cover Seals	4 pieces	

* Centrifugation immediately before use

5. Safety Notes

- 5.1 Avoid any skin and eye contact with Stop Solution and TMB. In case of contact, wash thoroughly with water.
- 5.2 Do not use the kit after the expiration date.
- 5.3 Do not mix or substitute reagents or materials from other kit lots or other sources.
- 5.4 Be sure to wear protective equipment such as gloves, masks and goggles during the experiment.
- 5.5 When using an automated plate washer, adding a 30 second soak period following the addition of Wash Buffer to improve assay precision

6. Sample Collection and Storage

- 6.1 Serum: Allow blood samples to clot for 30 minutes, followed by centrifugation for 15 minutes at 1000×g. Clear serum can be assayed immediately or aliquoted and stored at -20°C. Avoid repeated freeze-thaw cycles.
- 6.2 Plasma: Use EDTA, heparin, or citrate as an anticoagulant for plasma collection. Centrifuge for 15 minutes at 1000×g within 30 minutes of collection. The plasma can be assayed immediately or aliquoted and stored at -20°C. Avoid repeated freeze-thaw cycles.
- 6.3 Cell Culture Supernatant: Remove particulates by centrifugation for 5 minutes at 500×g and assay immediately or aliquot and store samples at ≤ -20°C. Avoid repeated freeze-thaw cycles.
- 6.4 Urine: Collect urine samples and centrifuge for 20 minutes at 1000×g. Collect the aqueous layer, assay immediately or aliquot and store samples at ≤ -20°C. Avoid repeated freeze-thaw cycles.

7. Regent Preparation

7.1 Wash Buffer (1X): If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Add 30 mL of Wash Buffer Concentrate(20X) to 570 mL deionized or distilled water to prepare 1X Wash Buffer.

7.2 Antibody Cocktail (1X): Dilute 100X capture antibody and 100X HRP-conjugated detection antibody using Detection Diluent prior to assay. Suggested 1:100 dilution: 50 µL 100X capture antibody + 50 µL 100X Detection Antibody, HRP-conjugated + 4,900 µL Detection Diluent. Mix gently but thoroughly.


7.3 Sample Dilution: Different samples should be diluted with corresponding Sample Diluent. The minimum required dilution factor was 1:2; consequently, no more than 25 µL of undiluted sample was added per well.

Samples may require further dilution if the readout values are higher than the highest standard OD reading. Variations in sample collection, processing and storage may affect the results of the measurement.

Recommended Dilution for different sample types: 1:4 or 1:8 is recommended for human serum and plasma; 1:2,000 or 1:4,000 is recommended for human cell culture supernatant; 1:8 or 1:16 is recommended for human urine; 1:8 or 1:16 is recommended for cynomolgus monkey serum and plasma; 1:512 or 1:1,024 is recommended for cynomolgus monkey cell culture supernatant.

7.4 Standard Serial Dilution:

Add 2 mL Sample Diluent PT 3-ef in protein standard.

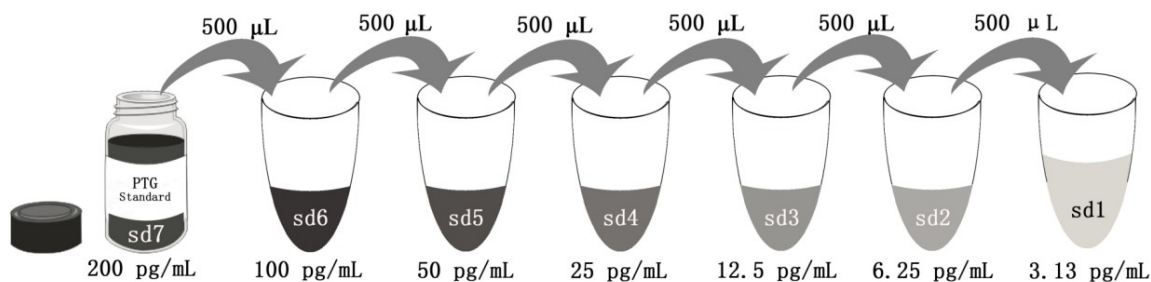

Add # µL of Standard diluted in the previous step	—	500 µL	500 µL	500 µL	500 µL	500 µL	500 µL
# µL of Sample Diluent PT 3-ef	2000 µL	500 µL	500 µL	500 µL	500 µL	500 µL	500 µL
	"sd7"	"sd6"	"sd5"	"sd4"	"sd3"	"sd2"	"sd1"

8. Assay Procedure Summary

Bring all reagents to room temperature before use (Detection antibody, HRP-conjugated antibody can be used immediately). To avoid cross-contamination, change pipette tips between additions of each standard level, between sample additions, and between reagent additions. Also, use separate reservoirs for each reagent.

8.1 Preset the layout of the microplate, including control group, standard group and sample group, take out the required number of microplate strips and return excess strips to the foil pouch containing the drying reagent pack and reseal; store at 4°C immediately. Microplate strips should be used in one week.

8.2 Add 50 µL standard or sample to appropriate wells. To avoid high background always add samples or standards to the well before the addition of antibody cocktail.

8.3 Add 50 µL 1× Antibody Cocktail solution (refer to Reagent Preparation 7.2) to each well. Seal plate with cover seal and incubate at 37°C on a microplate thermostatic shaker set at 400 rpm for 1 hour (incubate at 37°C for 2 hours is recommended if thermostatic shaker is not available) .

8.4 Wash

1) Gently remove the cover seal. Discard the liquid from wells by aspirating or decanting. Remove any residual solution by tapping the plate a few times on fresh paper towels.

2) Wash 4 times with 1× Wash Buffer, using at least 350-400 µL per well. Following the last wash, firmly tap plates on fresh towels 10 times to remove residual Wash Buffer. Avoid getting any towel fibers in the wells or wells drying out completely.


8.5 Add 100 µL TMB substrate solution to each well, protected from light. Incubate at 37°C on a microplate thermostatic shaker set at 400 rpm for 15 to 20 minutes. (Substrate Solution should remain colorless until added to the plate.)

8.6 Add 100 µL Stop Solution to each well in the same order as addition of the TMB substrate. Note: Avoid skin and eye contact with the Stop solution.

8.7 Read results immediately on a microplate reader at a wavelength of 450 nm. If possible, perform a double wavelength readout (450 nm and 630 nm).

8.8 Data analysis: Calculate the average of the duplicate readings (OD value) for each standard and sample, and subtract the average of the zero standard absorbance. Construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis, four-parameter logistic curve-fit (4-PL) analysis is recommended. If the samples have been diluted, the fitting result must be multiplied by the dilution factor used.


Procedure summary

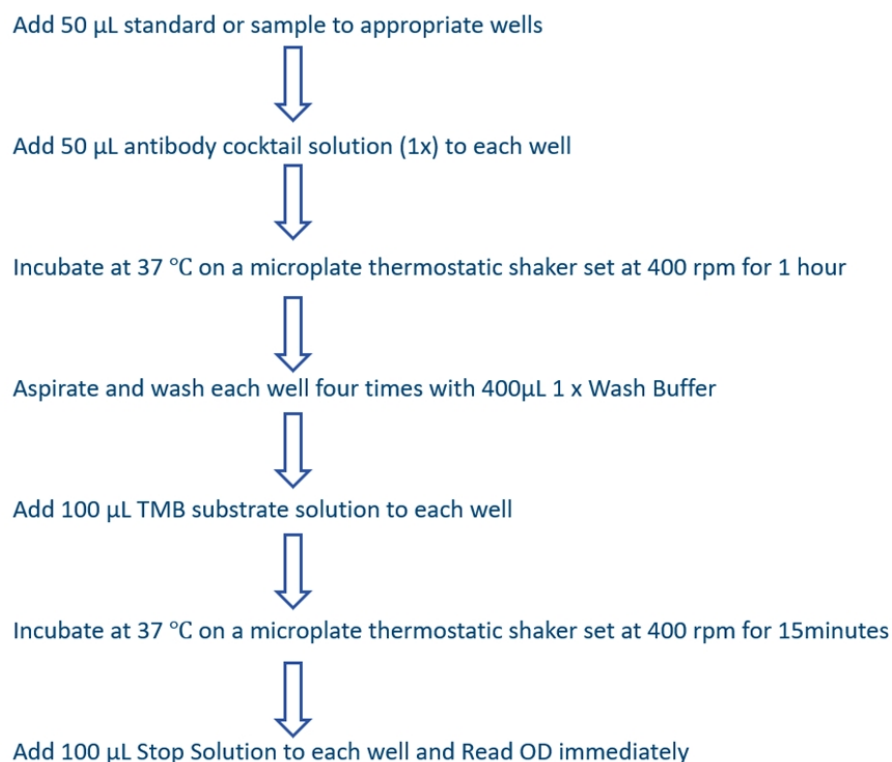

9. Validation Data

9.1 Standard curve

These standard curves are provided for demonstration only. A standard curve should be generated for each set of samples assayed.

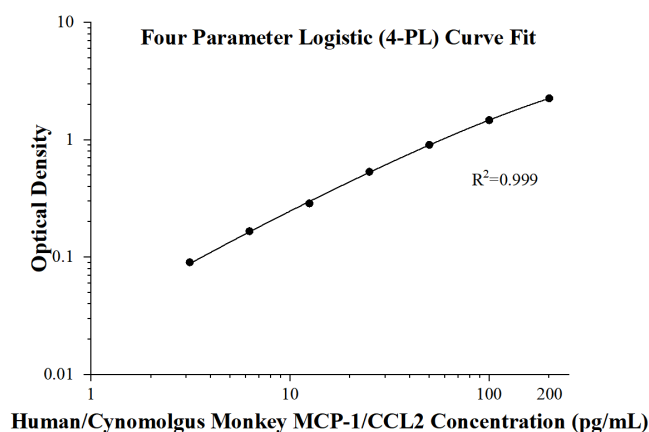

(pg/mL)	O.D	Average	Corrected
0	0.0226 0.0209	0.0218	-
3.13	0.1128 0.1119	0.1124	0.0906
6.25	0.1909 0.1859	0.1884	0.1667
12.5	0.3124 0.306	0.3092	0.2875
25	0.5625 0.5507	0.5566	0.5349
50	0.9254 0.9321	0.9288	0.9070
100	1.4914 1.4975	1.4945	1.4727
200	2.2706 2.2958	2.2832	2.2615

9.2 Precision

Intra-assay Precision (Precision within an assay) Three samples of known concentration were tested 8 times on one plate to assess intra-assay precision.

Inter-assay Precision (Precision between assays) Three samples of known concentration were tested in 16 separate assays to assess inter-assay precision.

Intra-assay Precision				
Sample	n	Mean (pg/mL)	SD	CV%
1	8	115.7	4.3	3.7
2	8	27.3	0.7	2.4
3	8	13.5	0.5	3.4

Inter-assay Precision				
Sample	n	Mean (pg/mL)	SD	CV%
1	16	110.3	6.4	5.8
2	16	26.3	1.3	5.0
3	16	12.9	0.8	6.4

9.3 Recovery

The recovery of human/cynomolgus monkey MCP-1/CCL2 spiked to three different levels throughout the range of the assay in various matrices was evaluated.

Sample Type		Average% of Expected	Range (%)
Human plasma	1:16	99	98-100
	1:32	100	97-102
Human cell culture supernatant	1:4,000	101	100-101
	1:8,000	100	99-101
Human urine	1:8	90	88-92
	1:16	98	97-98
Cynomolgus monkey serum	1:32	100	85-112
	1:64	94	93-97
Cynomolgus monkey cell culture supernatant	1:128	89	82-94
	1:256	88	84-89

9.4 Sample values

Plasma/Serum/Urine - human plasma, cynomolgus monkey serum and human urine samples were evaluated for the presence of MCP-1/CCL2 in this assay.

Sample Type	Mean (pg/mL)	Range (pg/mL)
Human plasma (n=16)	386.8	210.6-703.2
Cynomolgus monkey serum (n=8)	704.3	484.8-970.1
Human urine (n=8)	535.0	151.5-1,287.3

Cell culture supernatant:

Human peripheral blood mononuclear cells (1×10^6 cells/mL) were cultured in DMEM supplemented 10% fetal bovine serum, 5 μ M β -mercaptoethanol, 2 mM L-glutamine, 100 U/mL penicillin and 100 μ g/mL streptomycin sulfate. Cells were cultured unstimulated or stimulated with 10 μ g/mL PHA for 3 days. Aliquots of the cell culture supernates were removed and assayed for levels of MCP-1/CCL2.

Condition	Day 3 (ng/mL)
Unstimulated	49.2
Stimulated	274.3

Cynomolgus monkey peripheral blood mononuclear cells (1×10^6 cells/mL) were cultured in DMEM supplemented 10% fetal bovine serum, 5 μ M β -mercaptoethanol, 2 mM L-glutamine, 100 U/mL penicillin and 100 μ g/mL streptomycin sulfate. Cells were cultured unstimulated or stimulated with 10 μ g/mL PHA for 1 day, 3 days and 5 days. Aliquots of the cell culture supernates were removed and assayed for levels of MCP-1/CCL2.

Condition	Day 1 (ng/mL)	Day 3 (ng/mL)	Day 5 (ng/mL)
Unstimulated	7.3	37.9	28.2
Stimulated	11.0	43.6	57.6

9.5 Sensitivity

The minimum detectable dose of human/cynomolgus monkey MCP-1/CCL2 is 0.5 pg/mL. This was determined by adding two standard deviations to the concentration corresponding to the mean O.D. of 20 zero standard replicates.

9.6 Linearity

To assess the linearity of the assay, samples were diluted with the appropriate **Sample Diluent** to produce samples with values within the dynamic range of the assay.

(The human plasma was initially diluted 1:2. The human cell culture supernatant was initially diluted 1:1,000. The human urine was initially diluted 1:4. The cynomolgus monkey serum was initially diluted 1:4. The cynomolgus monkey cell culture supernatant was initially diluted 1:256.)

		Human plasma	Human cell culture supernatant	Human urine	Cynomolgus monkey serum	Cynomolgus monkey cell culture supernatant
1:2	Average% of Expected	100	100	100	100	100
	Range (%)	-	-	-	-	-
1:4	Average% of Expected	98	94	98	100	95
	Range (%)	92-103	92-96	94-102	98-101	94-96
1:8	Average% of Expected	99	92	102	102	90
	Range (%)	91-108	90-93	99-105	99-105	85-94
1:16	Average% of Expected	99	88	101	103	84
	Range (%)	87-110	86-89	98-105	101-106	78-90

9.7 Specificity

This assay recognizes natural and recombinant human/cynomolgus monkey MCP-1/CCL2.

The following factors prepared at 50 ng/mL were assayed and exhibited no cross-reactivity or interference.

Recombinant human:

MCP-2

MCP-3

MCP-4

GRO α

GRO β

IL-8

RANTES

Recombinant mouse:

JE/MCP-1

10. References

1. Sørensen, T L et al. European journal of neurology vol. 11,7 (2004): 445-9.
2. Kusano, Kengo Fukushima et al. Circulation journal : official journal of the Japanese Circulation Society vol. 68,7 (2004): 671-6.
3. Hayashida, K et al. Arthritis research vol. 3,2 (2001): 118-26.
4. Dimitrijevic, Oliver B et al. Journal of cerebral blood flow and metabolism : official journal of the International Society of Cerebral Blood Flow and Metabolism vol. 26,6 (2006): 797-810.
5. Mahad, Don J, and Richard M Ransohoff. Seminars in immunology vol. 15,1 (2003): 23-32.