

## Speedy™ Mouse LIX/CXCL5 One-Step ELISA Kit Datasheet

Please read it entirely before use

**Catalogue Number:** SE60078

**Size:** 96T

**Sensitivity:** 0.5 pg/mL

**Range:** 3.13-200 pg/mL

**Usage:** For the quantitative detection of mouse LIX/CXCL5 concentrations in serum, plasma, cell culture supernatant, urine and tissue lysate.


**This product is for research use only and not for use in human or animal therapeutic or diagnostic.**

<b>Table of content</b>	<b>page</b>
1. Background .....	3
2. Principle .....	3
3. Required Materials .....	3
4. Kit Components and Storage .....	4
5. Safety Notes .....	4
6. Sample Collection and Storage .....	5
7. Regent Preparation .....	6
8. Assay Procedure Summary .....	7
9. Validation Data .....	9
9.1 Standard curve .....	9
9.2 Precision .....	10
9.3 Recovery .....	10
9.4 Sample values .....	11
9.5 Sensitivity .....	11
9.6 Linearity .....	12
9.7 Specificity .....	12
10. References .....	12

## 1. Background

LPS-induced CXC chemokine (LIX) is a murine chemokine similar to two human chemokines, ENA-78 (CXCL5) and GCP-2 (CXCL6). Mouse LIX can be produced by many immune cells, such as macrophages, eosinophils, as well as non-immune cells including mesothelial cells, and fibroblasts. Increased serum LIX has been observed in obesity and insulin resistance in mice and humans and is associated with complications of diabetes including nephropathy and atherosclerosis. It is mainly produced when induced by LPS, IL-17 and/or TNF- $\alpha$ . According to the previous studies, cancer cell autonomous secretion of LIX is sufficient to drive infiltration of mature, protumorigenic neutrophils in a mouse model of non-small cell lung cancer (NSCLC).

## 2. Principle

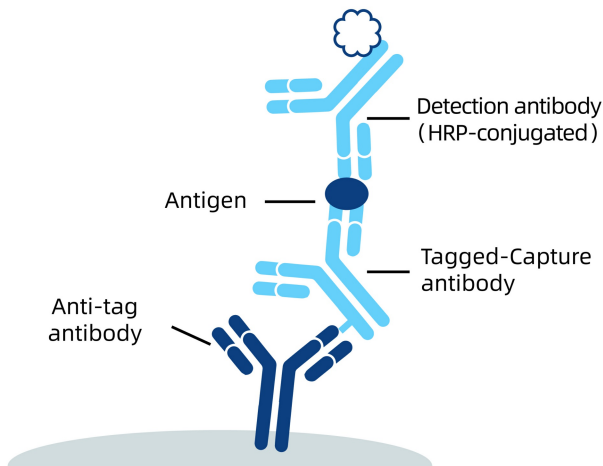

An anti-tag antibody is pre-coated onto the bottom of wells. After adding antigen or samples, Tagged-Capture antibody and HRP-conjugated detection antibody, a sandwich complex is formed in the solution. TMB acts as a HRP substrate, and the solution color will change from colorless to blue. A stop solution containing sulfuric acid turns the solution yellow. The color intensity is proportional to the quantity of bound protein, which is measurable at 450 nm with the correction wavelength set at 630 nm.

## 3. Required Materials

- 3.1 A microplate reader capable of measuring absorbance at 450 nm with the correction wavelength set at 630 nm.
- 3.2 Calibrated, adjustable precision pipettes and disposable plastic tips. A manifold multi-channel pipette is recommended for large assays.
- 3.3 Plate washer: automated or manual.
- 3.4 Absorbent paper towels.
- 3.5 Glass or plastic tubes to prepare standard and sample dilutions.
- 3.6 Beakers and graduated cylinders.
- 3.7 Log-log or semi-log graph paper or computer and software for ELISA data analysis. A four-parameter logistic (4-PL) curve-fit is recommended. Proteintech data analysis website, <https://www.ptgcn.com/products/elisa-kits/>.
- 3.8 Microplate thermostatic shaker.

## 4. Kit Components and Storage

<b>Microplate</b> - 96 well microplate precoated an anti-tag antibody (8 well × 12 strips)	1 plate	<b>Unopened Kit:</b> Store at 2-8°C for 6 months or -20°C for 12 months. <b>Opened Kit:</b> All reagents stored at 2-8°C for 7 days. <b>Please use a new standard for each assay.</b>
<b>Protein standard</b> - 400 pg/bottle; lyophilized	2 bottles	
<b>Capture antibody (100×)</b> - 60 µL/vial*	1 vial	
<b>Detection antibody, HRP-conjugated (100×)</b> - 60 µL/vial*	1 vial	
<b>Sample Diluent PT 5</b> - 30 mL/bottle. For mouse serum and plasma.	1 bottle	
<b>Sample Diluent PT 4B1</b> - 30 mL/bottle. For cell culture supernatant, urine and tissue lysate.	1 bottle	
<b>Detection Diluent</b> - 15 mL/bottle	1 bottle	
<b>Wash Buffer Concentrate (20×)</b> - 30 mL/bottle	1 bottle	
<b>Extraction Reagent</b> - 15 mL/bottle	1 bottle	
<b>Tetramethylbenzidine Substrate (TMB)</b> - 12 mL/bottle	1 bottle	
<b>Stop Solution</b> - 12 mL/bottle	1 bottle	
<b>Plate Cover Seals</b>	4 pieces	

\* Centrifugation immediately before use

## 5. Safety Notes

- 5.1 Avoid any skin and eye contact with Stop Solution and TMB. In case of contact, wash thoroughly with water.
- 5.2 Do not use the kit after the expiration date.
- 5.3 Do not mix or substitute reagents or materials from other kit lots or other sources.
- 5.4 Be sure to wear protective equipment such as gloves, masks and goggles during the experiment.
- 5.5 When using an automated plate washer, adding a 30 second soak period following the addition of Wash Buffer to improve assay precision

## 6. Sample Collection and Storage

6.1 Serum: Allow blood samples to clot for 30 minutes, followed by centrifugation for 15 minutes at 1000xg. Clear serum can be assayed immediately or aliquoted and stored at -20°C. Avoid repeated freeze-thaw cycles.

6.2 Plasma: Use EDTA, heparin, or citrate as an anticoagulant for plasma collection. Centrifuge for 15 minutes at 1000xg within 30 minutes of collection. The plasma can be assayed immediately or aliquoted and stored at -20°C. Avoid repeated freeze-thaw cycles.

6.3 Cell Culture Supernatant: Remove particulates by centrifugation for 5 minutes at 500xg and assay immediately or aliquot and store samples at  $\leq$  -20°C. Avoid repeated freeze-thaw cycles.

6.4 Urine: Collect urine samples and centrifuge for 20 minutes at 1000xg. Collect the aqueous layer, assay immediately or aliquot and store samples at  $\leq$  -20°C. Avoid repeated freeze-thaw cycles.

6.5 Tissue Lysate:

1) Rinse tissue with PBS, cut into 1-2 mm pieces.

2) Add protease inhibitor cocktail to the Extraction Reagent to a final concentration immediately prior to performing tissue lysis.

3) Add 1 mL of Extraction Reagent containing protease inhibitor cocktail per 100 mg tissue.

4) Homogenize the tissue completely using desired method on ice, Incubate on ice for 30 minutes, use ultrasound to break up the cells.

5) Centrifuge tissue homogenates at 10,000 x g for 5 minutes at 4°C. Collect the supernatant, assay immediately or aliquot and store at -20°C.

6) Measure the concentration of total protein in tissue homogenates using BCA assay.

7) Avoid protein degradation by performing all the above procedures on ice where possible.

## 7. Regent Preparation

**7.1 Wash Buffer (1X):** If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Add 30 mL of Wash Buffer Concentrate(20X) to 570 mL deionized or distilled water to prepare 1X Wash Buffer.


**7.2 Antibody Cocktail (1X):** Dilute 100X capture antibody and 100X HRP-conjugated detection antibody using Detection Diluent prior to assay. Suggested 1:100 dilution: 50  $\mu$ L 100X capture antibody + 50  $\mu$ L 100X Detection Antibody, HRP-conjugated + 4,900  $\mu$ L Detection Diluent. Mix gently but thoroughly.

**7.3 Sample Dilution:** Different samples should be diluted with corresponding Sample Diluent, samples may require further dilution if the readout values are higher than the highest standard OD reading. Variations in sample collection, processing and storage may affect the results of the measurement.

Recommended Dilution for different sample types: 1:200 or 1:400 is recommended for mouse serum and plasma; 1:2 to 1:32 is recommended for cell culture supernatant; 1:8 or 1:16 is recommended for urine; 1:128 or 1:256 is recommended for tissue lysate.

### 7.4 Standard Serial Dilution:

For mouse serum and plasma, add 2 mL Sample Diluent PT 5 in protein standard. For cell culture supernatant, urine and tissue lysate, add 2 mL Sample Diluent PT 4B1 in protein standard.

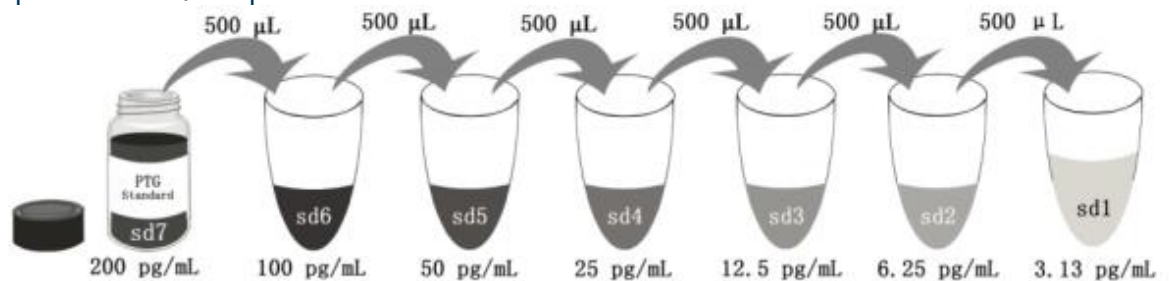

Add # $\mu$ L of Standard diluted in the previous step	—	500 $\mu$ L	500 $\mu$ L	500 $\mu$ L	500 $\mu$ L	500 $\mu$ L	500 $\mu$ L
# $\mu$ L of Sample Diluent PT 5 or PT 4B1	2000 $\mu$ L	500 $\mu$ L	500 $\mu$ L	500 $\mu$ L	500 $\mu$ L	500 $\mu$ L	500 $\mu$ L
	"sd7"	"sd6"	"sd5"	"sd4"	"sd3"	"sd2"	"sd1"

## 8. Assay Procedure Summary

Bring all reagents to room temperature before use (Detection antibody, HRP-conjugated antibody can be used immediately). To avoid cross-contamination, change pipette tips between additions of each standard level, between sample additions, and between reagent additions. Also, use separate reservoirs for each reagent.

8.1 Preset the layout of the microplate, including control group, standard group and sample group, take out the required number of microplate strips and return excess strips to the foil pouch containing the drying reagent pack and reseal; store at 4°C immediately. Microplate strips should be used in one week.

8.2 Add 50 µL standard or sample to appropriate wells. To avoid high background always add samples or standards to the well before the addition of antibody cocktail.

8.3 Add 50 µL 1× Antibody Cocktail solution (refer to Reagent Preparation 7.2) to each well. Seal plate with cover seal and incubate at 37°C on a microplate thermostatic shaker set at 400 rpm for 1 hour (incubate at 37°C for 2 hours is recommended if thermostatic shaker is not available) .

### 8.4 Wash

1) Gently remove the cover seal. Discard the liquid from wells by aspirating or decanting. Remove any residual solution by tapping the plate a few times on fresh paper towels.

2) Wash 4 times with 1× Wash Buffer, using at least 350-400 µL per well. Following the last wash, firmly tap plates on fresh towels 10 times to remove residual Wash Buffer. Avoid getting any towel fibers in the wells or wells drying out completely.

8.5 Add 100 µL TMB substrate solution to each well, protected from light. Incubate at 37°C on a microplate thermostatic shaker set at 400 rpm for 15 to 20 minutes. (Substrate Solution should remain colorless until added to the plate.)

8.6 Add 100 µL Stop Solution to each well in the same order as addition of the TMB substrate. Note: Avoid skin and eye contact with the Stop solution.

8.7 Read results immediately on a microplate reader at a wavelength of 450 nm. If possible, perform a double wavelength readout (450 nm and 630 nm).

8.8 Data analysis: Calculate the average of the duplicate readings (OD value) for each standard and sample, and subtract the average of the zero standard absorbance. Construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis, four-parameter logistic curve-fit (4-PL) analysis is recommended. If the samples have been diluted, the fitting result must be multiplied by the dilution factor used.

## Procedure summary

Add 50  $\mu$ L standard or sample to appropriate wells



Add 50  $\mu$ L antibody cocktail solution (1x) to each well



Incubate at 37  $^{\circ}$ C on a microplate thermostatic shaker set at 400 rpm for 1 hour



Aspirate and wash each well four times with 400 $\mu$ L 1 x Wash Buffer



Add 100  $\mu$ L TMB substrate solution to each well



Incubate at 37  $^{\circ}$ C on a microplate thermostatic shaker set at 400 rpm for 15minutes




Add 100  $\mu$ L Stop Solution to each well and Read OD immediately


## 9. Validation Data

### 9.1 Standard curve

These standard curves are provided for demonstration only. A standard curve should be generated for each set of samples assayed.

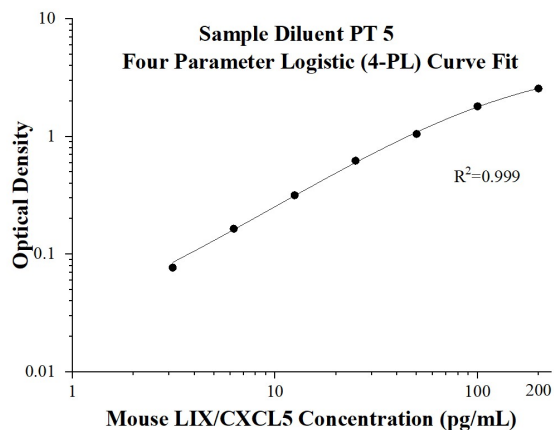

(pg/mL)	O.D	Average	Corrected
0	0.0104 0.0083	0.0094	-
3.13	0.0867 0.0858	0.0863	0.0769
6.25	0.1897 0.1581	0.1739	0.1646
12.5	0.3471 0.3056	0.3264	0.3170
25	0.6293 0.6355	0.6324	0.6231
50	1.0331 1.091	1.0621	1.0527
100	1.9307 1.6997	1.8152	1.8059
200	2.623 2.5242	2.5736	2.5643

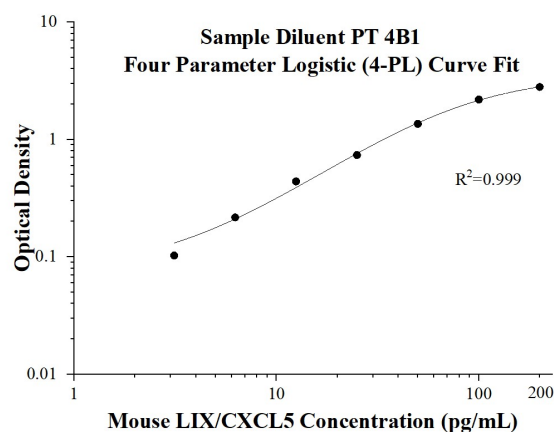

(pg/mL)	O.D	Average	Corrected
0	0.0242 0.0196	0.0219	-
3.13	0.1221 0.1269	0.1245	0.1026
6.25	0.2353 0.2423	0.2388	0.2169
12.5	0.417 0.5061	0.4616	0.4397
25	0.759 0.7603	0.7597	0.7378
50	1.3924 1.369	1.3807	1.3588
100	2.2 2.2187	2.2094	2.1875
200	2.8387 2.8046	2.8217	2.7998

## 9.2 Precision

**Intra-assay Precision** (Precision within an assay) Three samples of known concentration were tested 8 times on one plate to assess intra-assay precision.

**Inter-assay Precision** (Precision between assays) Three samples of known concentration were tested in 16 separate assays to assess inter-assay precision.

Intra-assay Precision				
Sample	n	Mean (pg/mL)	SD	CV%
1	8	98.6	1.6	1.6
2	8	26.2	0.8	3.1
3	8	14.7	0.3	2.0

Inter-assay Precision				
Sample	n	Mean (pg/mL)	SD	CV%
1	16	95.7	4.0	4.2
2	16	26.2	0.9	3.4
3	16	14.4	0.4	2.8

## 9.3 Recovery

The recovery of mouse LIX/CXCL5 spiked to three different levels throughout the range of the assay in various matrices was evaluated.

Sample Type		Average% of Expected	Range (%)
Mouse serum	1:800	96	87-103
	1:1,600	106	101-113
Cell culture supernatant	1:8	102	96-110
	1:16	100	96-102
Urine	1:32	87	84-88
	1:64	105	98-117
Tissue lysate	1:128	97	76-120
	1:256	116	114-118

## 9.4 Sample values

**Mouse serum/Urine** - Mouse serum and urine samples were evaluated for the presence of mouse LIX/CXCL5 in this assay.

Sample Type	Mean (ng/mL)	Range (ng/mL)
Mouse serum (n=16)	15.5	13.4-18.7

Sample Type	Mean (pg/mL)	Range (pg/mL)
Urine (n=8)	342.1	25.0-1,449.3

**Cell culture supernatant** - Mouse lung (1 lung, 1-2 mm pieces) tissue were cultured for 1 day in RPMI1640 plus 15% fetal bovine serum and stimulated with 1 µg/mL LPS. An aliquot of cell culture supernatants was removed, assayed for mouse LIX/CXCL5.

Condition	Day 1 (pg/mL)
Unstimulated	53.4
Stimulated	924.6

### Tissue lysate

	Mouse LIX/CXCL5 (ng/mL)	Total protein (mg/mL)
Mouse lung tissue lysate	2.6	5.0
Mouse spleen tissue lysate	7.4	6.4

## 9.5 Sensitivity

The minimum detectable dose of mouse LIX/CXCL5 is 0.5 pg/mL. This was determined by adding two standard deviations to the concentration corresponding to the mean O.D. of 20 zero standard replicates.

## 9.6 Linearity

To assess the linearity of the assay, samples were diluted with the appropriate **Sample Diluent** to produce samples with values within the dynamic range of the assay.

(The mouse serum was initially diluted 1:100. The cell culture supernatant was initially diluted 1:8. The urine was initially diluted 1:4. The tissue lysate was initially diluted 1:64.)

		Mouse serum (Sample Diluent PT 5)	Cell culture supernatant (Sample Diluent PT 4B1)	Urine (Sample Diluent PT 4B1)	Tissue lysate (Sample Diluent PT 4B1)
1:2	Average% of Expected	100	100	100	100
	Range (%)	-	-	-	-
1:4	Average% of Expected	102	100	115	101
	Range (%)	93-111	95-106	111-119	100-102
1:8	Average% of Expected	104	99	120	99
	Range (%)	90-118	89-109	119-121	97-101
1:16	Average% of Expected	97	102	126	96
	Range (%)	81-114	89-114	124-128	93-99

## 9.7 Specificity

This assay recognizes natural and recombinant mouse LIX/CXCL5.

The following factors prepared at 50 ng/mL were assayed and exhibited no cross-reactivity or interference.

Recombinant human:

CXCL5/ENA-78

CXCL6/GCP-2

Recombinant mouse:

CXCL1/KC

CXCL2/MIP-2

Recombinant rat:

LIX

## 10. References

1. Jeffrey B. Smith. et al. (2002) Immunogenetics. 54:599-603
2. Gopalakrishnan, A. et al. (2019) Infect Immun. 03 ;87(3)
3. Wang, CY. et al. (2019) Med Sci Monit.17;25:5299-5305
4. Mylonas, KJ. et al. (2017) J Endocrinol. 06;233(3):315-327
5. Chave. et al. (2009) Cell Metab. 9, 339-349
6. Nunemaker. et al. (2014) J. Endocrinol. 222, 267-276
7. Francesca Simoncello. et al. (2022) Oncoimmunology.11(1) :2059876